

# SCIENTIFIC REVIEW



 **AMINO**Gram



**20 years of expertise  
and continuous innovation.**

# Table of contents

|   |    |
|---|----|
| ■ Principles of Bioelectrical Impedance Analysis (BIA).....                               | 4  |
| ■ Application domains of bioelectrical impedance analysis.....                            | 5  |
| Technological choices of Biody Xpert <sup>z</sup> M3 with tetrapolar measurement.....     | 6  |
| Validation of seated and supine measurement versus DEXA.....                              | 7  |
| Comparison of results obtained between Biody Xpert <sup>z</sup> M and DEXA.....           | 8  |
| ■ Single-frequency BIA (SF), multi-frequency BIA (MF-BIA) and spectroscopy BIA (BIS)..... | 9  |
| Selection of studies with abstracts (accessible DOIs).....                                | 11 |
| Complete list of published studies (updated: June 26, 2025).....                          | 11 |
| ■ Partners and user centers.....  | 13 |
| ■ Literature notes.....   | 14 |

# Principles of Bioelectrical Impedance Analysis (BIA)

BIA is a non-invasive and painless technique for analyzing body composition.

It consists of delivering one or more very low intensity currents to measure the resistance of tissues to the passage of the current.

These measurements make it possible to obtain values of resistance, reactance, and impedance.

More precisely:

- › resistance is related to the state of hydration (transitive resistance)
- › reactance is related to the quantity and integrity of the cell membrane (capacitive resistance)<sup>1</sup>
- › impedance, as for it, is calculated from these two parameters according to the following formula:

$$Z(\omega) = R(\omega) + j \times Xc(\omega)$$

Where **Z** represents impedance, **R** resistance, **Xc** reactance, **j** the imaginary component of the signal, and **ω** the current frequency.

It is then used within predictive equations to evaluate body composition, including, for example, hydration, skeletal muscle mass, or fat mass.

In addition to body composition parameters, BIA also allows obtaining raw parameters related to overall health status and systemic inflammation level, such as phase angle and impedance ratio<sup>2,3</sup>.

From a technical point of view, these bioelectrical data can be obtained by two measurement modes using 4 electrodes (tetrapolar) or 8 electrodes (octopolar), which will be connected to the hand and foot.



# Application domains of bioelectrical impedance analysis

Currently, BIA is used during clinical management, health status monitoring, or during physical preparation of athletes to:

- detect possible pathological imbalances in body composition or situations at risk of developing these imbalances,
- guide clinical, nutritional and/or sports management targeting body composition,
- evaluate the effectiveness of this management to reorient it if necessary.

The image displays three screenshots of scientific articles from the European Society for Clinical Nutrition (ESPEN) website. The first article is 'Bioelectrical impedance analysis—part I: review of principles and methods' (2008), the second is 'Bioelectrical impedance analysis—part II: utilization in clinical practice' (2008), and the third is 'ESASO consensus statement' (2010) regarding sarcopenic obesity. Each screenshot shows the article's title, authors, abstract, and keywords.

In 2004, the European Society for Clinical Nutrition (ESPEN) issued recommendations for the use of BIA in healthy subjects and patients with chronic pathologies, according to a tetrapolar mode and the equations developed for it, for routine clinical use<sup>4,5</sup>.

It is notably recommended for the detection of undernutrition<sup>6</sup> and sarcopenia<sup>7</sup>, as well as in the diagnosis of obesity<sup>8</sup> and sarcopenic obesity<sup>9</sup>.

In a sports context, it is also used for monitoring body composition during physical preparation, and in prevention of chronic energy restriction syndrome (RED-S)<sup>10</sup>.

Generally, the parameters used during management include fat-free mass, fat mass, skeletal muscle mass (total and segmental), as well as body hydration and the balance between intra- and extracellular compartments.

Compared to other techniques, BIA stands out for its ease of use, speed of measurement, convenience for the subject, and low cost<sup>11</sup>.

Like any method, however, it presents certain limitations, particularly in clinical contexts where the hydration status is strongly disturbed. These specific situations require an adapted interpretation, by cross-referencing clinical data with the results obtained.

## Technological choices of Biody Xpert<sup>TM</sup>3 with tetrapolar measurement

Tetrapolar measurement consists of placing two pairs of electrodes on the hand and foot: one emits a low-intensity electric current, the other measures the generated voltage. This allows obtaining the bioelectrical data necessary for evaluating body composition.

As indicated in part 1, this measurement mode is recommended in the literature for clinical management, as the equations used and validated are specifically adapted to tetrapolar measurement. In this context, Aminogram has chosen to use predictive equations from the scientific literature, validated against reference methods:

- › An equation modified from that of Kyle et al.<sup>12</sup> for fat-free mass;
- › The Kushner & Schoeller<sup>13</sup> equation for total body water volume;
- › The Deurenberg et al. equation for extracellular water volume;
- › The Kyle et al.<sup>15</sup> equation for appendicular skeletal muscle mass.

Bone mineral content is estimated from an internally developed algorithm. Other body compartments are deduced from compartmental modeling. For example, if total water and extracellular water are known, intracellular water can be calculated using the formula:

Intracellular water = Total water - Extracellular water.



When a measurement is performed in a supine position, one limitation of this measurement mode is the necessity to maintain a minimum time of several minutes in this position before performing the measurement, in order to allow for a balance of body fluids following the change in posture, and thus obtain optimal results. This waiting time can limit the use of the technique in a routine care context, due to a measurement duration that may conflict with the available consultation time.

Furthermore, the use of self-adhesive electrodes in the form of consumables implies a significant financial cost, particularly for hospital structures performing a large number of measurements, which can also limit the use of the technique. Based on this observation, Aminogram chose to develop a device offering two possibilities: a supine measurement with cables and self-adhesive electrodes, or a seated measurement with integrated electrodes, allowing for the avoidance of consumables and reducing measurement time. The result of this development is the Biody Xpert<sup>TM</sup> range, designed to adapt to clinical constraints while guaranteeing data quality.

# Validation of seated and supine measurement versus DEXA

The measurement position and electrode placement are determining parameters in bioelectrical impedance analysis. If the measured bioelectrical data (resistance, reactance, impedance) do not vary depending on the position, the body composition results can be considered comparable.

A study conducted by the National Institute of Physical Education of Catalonia (INEFc) on 30 healthy subjects evaluated the precision of the Biody Xpert<sup>ZM3</sup><sup>16</sup> in seated and supine positions (published in Measurement (IF: 5,6)). The 50 kHz measurements were very close:

## Key data from the INEFC study (2024):

Only 3.7 Ω average impedance difference between seated and supine positions.  
 Average deviation from DEXA: 0.3 to 0.8 kg depending on the parameters.

|                   | Seated         | Supine         |
|-------------------|----------------|----------------|
| <b>Resistance</b> | 486,2 ± 51,5 Ω | 489,5 ± 49,7 Ω |
| <b>Reactance</b>  | 60,9 ± 6,3 Ω   | 64,3 ± 7,5 Ω   |
| <b>Impedance</b>  | 493,7 ± 50,0 Ω | 490,0 ± 51,7 Ω |

Bland-Altman analysis indicates a mean difference of:

- › 3,3 Ω for resistance
- › 3,3 Ω for reactance
- › 3,7 Ω for impedance

Lin's concordance coefficient confirms very good consistency:

- › 0,92 for resistance
- › 0,79 for reactance
- › 0,92 for impedance

Body composition data were also compared with those obtained by DEXA:

|               | Fat-free mass | Lean mass     | Fat mass      |
|---------------|---------------|---------------|---------------|
| <b>Supine</b> | 62,8 ± 4,7 kg | 59,9 ± 4,5 kg | 16,3 ± 5,2 kg |
| <b>Seated</b> | 62,9 ± 5,5 kg | 60,0 ± 5,3 kg | 16,3 ± 4,6 kg |

The deviations from DEXA were small:

- › Fat-free mass: 0.6 kg (supine), 0.8 kg (seated)
- › Lean mass: 0,8 kg / -0,1 kg
- › Fat mass: 0,3 kg / 0,4 kg

These results confirm the equivalence of measurements between seated and supine positions, as well as good agreement with DEXA. Although the data concern a limited sample, they provide solid evidence supporting the reliability of the method, and open the way for further studies on larger populations.

# Comparison of results obtained between Biody Xpert<sup>TM</sup> and DEXA

To reinforce these results and broaden their scope, Aminogram compiled data from 234 subjects representative of the general population. These comparisons between the Biody Xpert II and DEXA were carried out as part of the Post-Marketing Clinical Follow-up (SCAC).

The concordance between the two techniques was evaluated according to recognized statistical methods: mean bias (mean difference) according to Bland-Altman, and intraclass correlation coefficient (ICC).

The results obtained confirm strong consistency between the two approaches for the four parameters analyzed: fat-free mass, fat mass, appendicular skeletal muscle mass, and bone mineral content (see figure below).

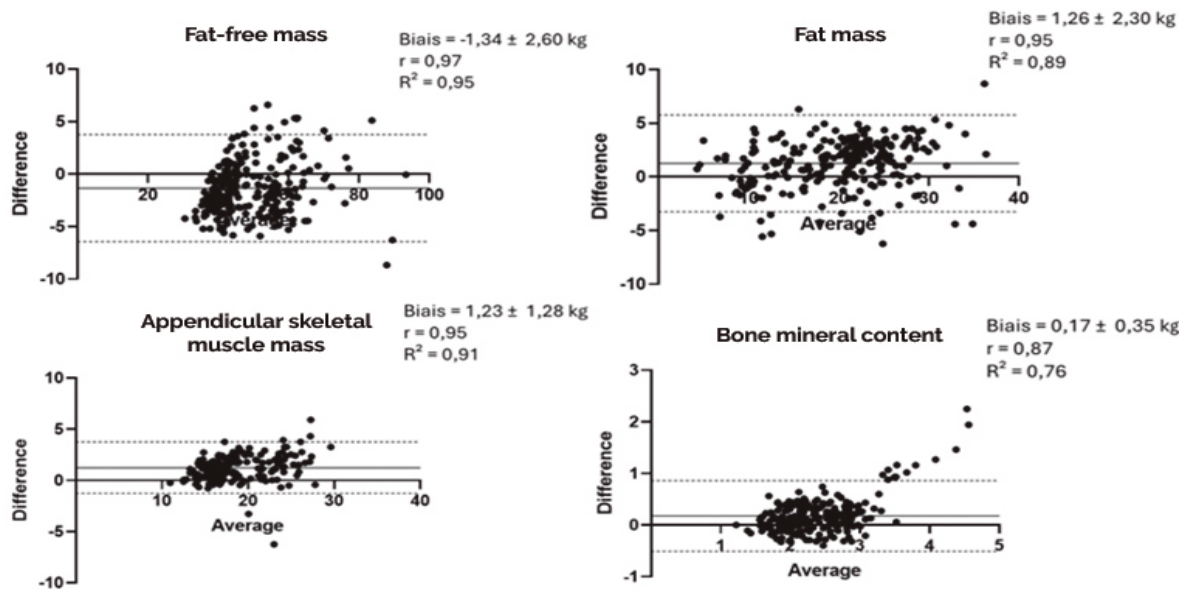


Figure: Bland-Altman plot of results obtained by the Biody XpertZMII and DEXA for fat-free mass, fat mass, appendicular skeletal muscle mass and bone mineral content. The intraclass correlation coefficient  $r$  and regression coefficient  $R^2$  are also given for each parameter.

The mean difference for fat-free mass, fat mass, and appendicular skeletal muscle mass is slightly greater than 1 kg with  $r$  values much higher than 0.90, indicating excellent concordance between the two techniques. For bone mineral content, the mean bias obtained is 170 grams with an  $r$  slightly lower than that of the other three parameters but which, nevertheless, indicates very good concordance between the two techniques for this parameter. It is interesting to observe that about ten points are outside the limits of the 95% confidence interval, i.e., the dashed lines, indicating a significant difference between the two techniques for these individuals. These correspond to rugby players who are characterized by extremely high bone density, caused by the stresses of their sport. As a technique, DEXA is sensitive to bone mineral density, unlike BIA, thus explaining the observed differences for these individuals.

In conclusion, these data show that for these 4 parameters, the Biody Xpert<sup>TM</sup>II, and the Biody Xpert<sup>TM</sup>3 by extension, demonstrate equivalence in the results obtained compared to DEXA in the general population.



# Single-frequency BIA (SF), multi-frequency BIA (MF-BIA) and spectroscopy BIA (BIS)

The first BIA devices were single-frequency, meaning they used a single current at a frequency of 50 kHz. They relied on prediction equations and reference values based on resistance, reactance, or impedance. The main limitation of this approach lies in its inability to precisely evaluate extracellular water volume and therefore the distribution between intra- and extracellular compartments. Indeed, at 50 kHz, the current passes through cell membranes, which prevents specifically targeting the extracellular compartment. This type of measurement has notably been used in early devices such as the R/L Systems Quantum II, considered a historical reference in the development of prediction equations.



R/L Systems Quantum II

The evaluation of the extracellular compartment is made possible by using low-frequency currents (below 7 kHz), which are unable to cross cell membranes<sup>17</sup>. So on this basis, multi-frequency devices have been developed, using at least three frequencies: a low one (generally 5 kHz), an intermediate one (50 kHz) and a high one (100 or 200 kHz). Their main advantage is to allow a distinct estimation of total water and extracellular water, via algorithms combining the data obtained at 5 and 50 kHz. These devices also provide access to equations validated in the literature, usable at 50 kHz. The introduction of a third frequency also makes it possible to calculate the impedance ratio (impedance at 200 kHz / impedance at 5 kHz), a marker associated with systemic inflammation<sup>3, 18</sup>.

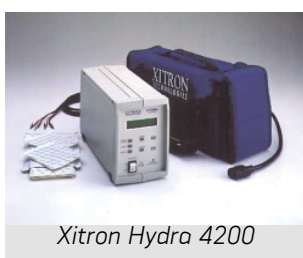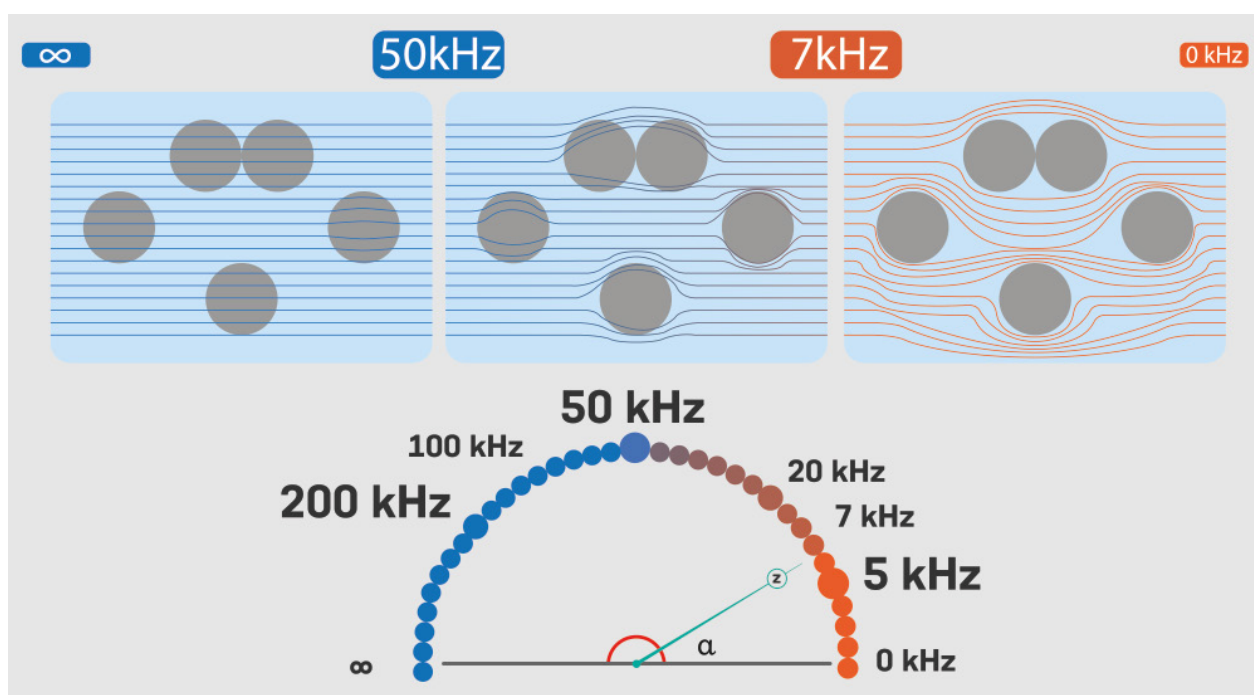

Xitron Hydra 4200

The most advanced reference devices, such as the Xitron Hydra 4200, rely on a spectroscopic approach. This consists of scanning a wide spectrum of frequencies—from very low to very high—to finely analyze the electrical properties of body tissues. The Body Xpert ZM3 fully aligns with this approach, with an analysis across 54 frequencies ranging from 1 kHz to 1000 kHz, including the lowest frequencies (1, 2, 3, and 4 kHz). This specificity makes it the only portable bio-impedance device with spectroscopy to provide

measurements at these frequencies, which are particularly sensitive to extracellular compartments.

Processing this data allows for the generation of a Cole-Cole curve, shown below, whose consistency between theoretical modeling (curve) and measured points guarantees the quality of the measurement.

Thanks to this analytical precision, it becomes possible to estimate three fundamental resistances associated with the body's water compartments:

| Estimated parameter                   | Physiological meaning                                  |
|---------------------------------------|--|
| Resistance at 0 Hz ( $R_0$ )          | Corresponds to extracellular water (outside cells)     |
| Intracellular resistance              | Reflects fluids contained inside cells                 |
| Resistance at infinity ( $R_\infty$ ) | Estimation of total body water (intra + extracellular) |

These data make it possible to feed more reliable body composition prediction equations than those based on a single frequency at 50 kHz, and adapted to a diversity of populations<sup>19</sup>.

Furthermore, several recent studies show that certain parameters extracted from spectroscopic analysis are correlated with major clinical indicators, notably:

- › insulin resistance<sup>20</sup>,
- › membrane permeability and exchanges<sup>21</sup>,
- › or the functional and architectural quality of skeletal muscle<sup>22, 23</sup>.

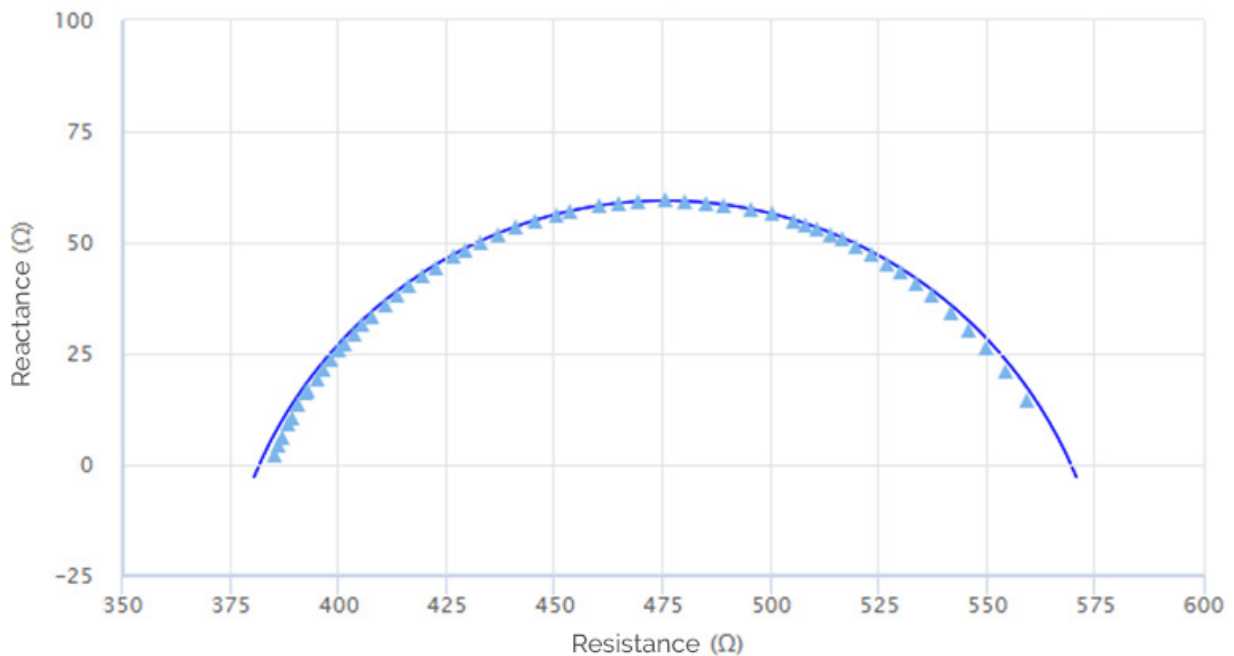


Figure: Graphical representation of Cole-Cole modeling. Each triangle represents a BIA data measurement at a precise frequency, over a range of 1 to 1000 kHz. The solid line represents the obtained Cole-Cole modeling. The position of the triangles relative to the Cole-Cole modeling allows for controlling the quality of the measurement.

# Studies conducted with our devices

## Selection of studies with abstracts (accessible DOIs)

Espasa-Labrador, Javier, Álex Cebrián-Ponce, Raúl Galindo-López, et al. « Intra-Rater Reliability and Agreement of a Portable Bioelectrical Impedance Analysis Device for Body Composition Assessment ». *Measurement* 259 (février 2026): 119550. <https://doi.org/10.1016/j.measurement.2025.119550>.

Imbert, Jean-Pierre, Axel Barbaud, Sian Stevens, Craig Miller, Hilary Peace, Helene Rossin, Alain Letourneur, Philip Bryson, Bo Damsgaard, et Costantino Balestra. « Evaluation of North Sea Saturation Procedures through Divers Monitoring ». *International Maritime Health* 75, no 2 (2024): 89 102. [https://journals.viamedica.pl/international\\_maritime\\_health/article/view/99606/78297](https://journals.viamedica.pl/international_maritime_health/article/view/99606/78297).

Maccarone, Maria Chiara, Daniele Coraci, Andrea Bernini, Nicola Sarandria, Marta Rossella Valente, Anna Chiara Frigo, Yannis Dionysiotis, et Stefano Masiero. « Sarcopenia Prevalence and Association with Nutritional Status in Cohort of Elderly Patients Affected by Musculoskeletal Concerns: A Real-Life Analysis ». *Frontiers in Endocrinology* 14 (26 juin 2023). <https://doi.org/10.3389/fendo.2023.1194676>.

Martínez-Rodríguez, Alejandro, Lorena Vidal-Martínez, María Martínez-Olcina, Laura Miralles-Amorós, Juan Antonio Sánchez-Sáez, Domingo Jesús Ramos-Campo, Javier Sánchez-Sánchez, et al. « Study the Effect of an Innovative Educational Program Promoting Healthy Food Habits on Eating Disorders, Mediterranean Diet Adherence and Body Composition in University Students ». *Healthcare* 11, no 7 (janvier 2023): 965. <https://doi.org/10.3390/healthcare11070965>.

Tapasco-Tapasco, L. O., C. A. Gonzalez-Correa, et A. Letourneur. « Phase Angle and Impedance Ratio as Meta-Inflammation Biomarkers after a Colon Cleansing Protocol in a Group of Overweight Young Women ». *Physiological Measurement* 45, no 5 (mai 2024): 055021. <https://doi.org/10.1088/1361-6579/ad46df>.

## Complete list of published studies (updated: June 26, 2025)

Barbry, Alexis, Annie Carton, Marjorie Bernier, Hervé Ovigneur, et Jérémy Bernard Coquart. « Does Brief Mindfulness Intervention Increase Performance? An Exploratory Study ». *International Journal of Sports Medicine*, 22 février 2025, a-2544-7523. <https://doi.org/10.1055/a-2544-7523>.

Barbry, Alexis, Annie Carton, Hervé Ovigneur, et Jérémy Coquart. « Effects of an 8-week of brief mindfulness meditation combined with a running programme on physical performances and health in runners: a randomized controlled study », 2023. <https://laas.hal.science/UREPSSS/hal-04161969v1>.

Bauduer, F., C. Monchaux, M. -L. Burtin, B. Dubroca, et J. -P. Mathieu. « Déséquilibres biochimiques, déshydratation, récupération et rugby professionnel – données du suivi longitudinal de la Ligue nationale de rugby et de l'exploration par bioimpédance multifréquence ». *Science & Sports* 26, no 1 (1 février 2011): 19 24. <https://doi.org/10.1016/j.scispo.2010.08.003>.

Becerril Alarcón, Yízel, Fernando Bastida González, Isidro Roberto Camacho Beiza, Eduardo Dávila González, José Alfonso Cruz Ramos, Alejandra Donají Benítez Arciniega, Roxana Valdés Ramos, et Alexandra Estela Soto Piña. « Association of GSTT1, GSTM1 and GSTP1 (Ile105Val) mRNA Expression with Cardiometabolic Risk Parameters in Women with Breast Cancer and Comorbidities ». *Cardiogenetics* 12, no 3 (septembre 2022): 235 45. <https://doi.org/10.3390/cardiogenetics12030022>.

Charatsi, A. M., P. Dusser, R. Freund, G. Maruani, H. Rossin, A. Boulier, M. Le Bourgeois, et al. « Bioelectrical Impedance in Young Patients with Cystic Fibrosis: Validation of a Specific Equation and Clinical Relevance ». *Journal of Cystic Fibrosis: Official Journal of the European Cystic Fibrosis Society* 15, no 6 (novembre 2016): 825 33. <https://doi.org/10.1016/j.jcf.2016.05.004>.

Cordova-Manzo, Jesus Fausto, Gabriela Flores-Mondragon, Gabriel Vega-Martínez, Cinthya L. Toledo-Peral, Arturo Vera-Hernández, et Lorenzo Leija-Salas. « Hydration Status During the Micturition Cycle Using Bioimpedance for Bladder Monitoring: A Pilot Study ». *Consulté le 21 février 2025*. <https://ieeexplore.ieee.org/document/10770905>.

Cuvelier, S., C. Goetgheluck-Villaron, M. Cohen, A. Tallet, M. Berline, J. M. Boher, S. Jowett, et al. « Aqua polo: Preliminary feasibility and efficacy study of a programme of adapted, supervised water polo to reduce fatigue and improve women's psychological and social recovery after breast cancer treatment: A mixed-methods design ». *Contemporary Clinical Trials Communications* 33 (1 juin 2023): 101120. <https://doi.org/10.1016/j.conctc.2023.101120>.

Donaciano-Domínguez, Jm, Id Salinas-Velarde, Y Becerril-Alarcón, et Ae Soto-Piña. « Phase angle variation and cellular hydration associated with GSTP1 gene polymorphisms in women with breast cancer ». *Journal of Physics: Conference Series* 3014, no 1 (1 mai 2025): 012013. <https://doi.org/10.1088/1742-6596/3014/1/012013>.

Espasa-Labrador, Javier, Álex Cebrián-Ponce, Raúl Galindo-López, et al. « Intra-Rater Reliability and Agreement of a Portable Bioelectrical Impedance Analysis Device for Body Composition Assessment ». *Measurement* 259 (février 2026): 119550. <https://doi.org/10.1016/j.measurement.2025.119550>.

Garduño Alanis, Adriana, Yízel Becerril Alarcón, Betsy Corina Sosa García, Lizbeth Morales González, Ángeles Leyda Avilés García, Blanca Guadalupe Alvarado Bravo, et Hugo Mendieta Zerón. « Depression as a Predictor of Sleep Quality in Health Workers Who Faced the COVID-19 Pandemic in Mexico », 10 octobre 2023. <http://ri.uaemex.mx/handle/20.500.11799/139260>.

Gianesini, Sergio, Joseph D. Raffetto, Giovanni Mosti, Elisa Maietti, Maria Grazia Sibilla, Paolo Zamboni, et Erica Menegatti. « Volume Control of the Lower Limb with Graduated Compression during Different Muscle Pump Activation Conditions and the Relation to Limb Circumference Variation ». *Journal of Vascular Surgery: Venous and Lymphatic Disorders* 8, no 5 (septembre 2020): 814 20. <https://doi.org/10.1016/j.jvsv.2019.12.073>.

González-Correa, C. A., S. A. Jaimes, et J. I. Cárdenas-Jiménez. « Preliminary Study on Parameterization of Raw Electrical Bioimpedance Data with 3 Frequencies ». *Scientific Reports* 12, no 1 (3 juin 2022): 9292. <https://doi.org/10.1038/s41598-022-13299-7>.

- Gouin, Emmanuel, Costantino Balestra, Jeremy Orsat, Emmanuel Dugrenot, et Erwan L'Her. « Pulmonary Effects of One Week of Repeated Recreational Closed-Circuit Rebreather Dives in Cold Water ». *Medicina* 59, no 1 (janvier 2023): 81. <https://doi.org/10.3390/medicina59010081>.
- Hayotte, Meggy, Antonio Iannelli, Véronique Nègre, Christian Pradier, Pierre Théroutan, Alain Fuch, Odile Diagona, et al. « Effects of technology-based physical activity interventions for women after bariatric surgery: study protocol for a three-arm randomised controlled trial ». *BMJ Open* 11, no 7 (30 juillet 2021): e046184. <https://doi.org/10.1136/bmjopen-2020-046184>.
- Huguel, Benjamin, Thibaud Vaugrenard, Ludivine Saby, Lionel Benhamou, Sébastien Arméro, Élise Camilleri, Aida Langar, Quentin Alitta, Michel Grino, et Frédérique Retornaz. « Feasibility and Acceptability of a Self-Measurement Using a Portable Bioelectrical Impedance Analysis, by the Patient with Chronic Heart Failure, in Acute Decompensated Heart Failure ». *Geriatric Et Psychologie Neuropsychiatrie Du Vieillessement* 16, no 2 (1 juin 2018): 145-54. <https://doi.org/10.1684/pnv.2018.0730>.
- Hurtado, B, E Colina, et C.H. Gonzalez-Correa. « Concordance between dual indirect methods for assessing fat percentage ». *Journal of Electrical Bioimpedance* 15, no 1 (s. d.): 26-32. <https://doi.org/10.2478/joeb-2024-0004>.
- Imbert, Jean-Pierre, Axel Barbaud, Sian Stevens, Craig Miller, Hilary Peace, Helene Rossin, Alain Letourneur, Philip Bryson, Bo Damsgaard, et Costantino Balestra. « Evaluation of North Sea Saturation Procedures through Divers Monitoring ». *International Maritime Health* 75, no 2 (2024): 89-102. [https://journals.viamedica.pl/international\\_maritime\\_health/article/view/99606/78297](https://journals.viamedica.pl/international_maritime_health/article/view/99606/78297).
- Lachguer, Sara, Miloud Chakit, Jhadiel Kossou, Hasna Kachache, Boujdi Rachid, Amina Bouziani, et Hasnae Benkirane. « OBESITY AND BODY COMPOSITION DETERMINED BY BIOIMPEDANCE-METRY IN MOROCCAN ADULT POPULATION ». *Community practitioner: the journal of the Community Practitioners' & Health Visitors' Association* 21 (6 juillet 2024): 7. <https://doi.org/10.5281/zenodo.12669994>.
- Leyva-Vela, Belén, María Martínez-Olcina, Nuria Asencio-Mas, Manuel Vicente-Martínez, Bernardo José Cuestas-Calero, Piotr Matos, et Alejandro Martínez-Rodríguez. « Integrated Multivariate Predictive Model of Body Composition and Lipid Profile for Cardiovascular Risk Assessment ». *Journal of Clinical Medicine* 14, no 3 (janvier 2025): 781. <https://doi.org/10.3390/jcm14030781>.
- Maccarone, Maria Chiara, Daniele Coraci, Andrea Bernini, Nicola Sarandria, Marta Rossella Valente, Anna Chiara Frigo, Yannis Dionysiotis, et Stefano Masiero. « Sarcopenia Prevalence and Association with Nutritional Status in Cohort of Elderly Patients Affected by Musculoskeletal Concerns: A Real-Life Analysis ». *Frontiers in Endocrinology* 14 (26 juin 2023). <https://doi.org/10.3389/fendo.2023.1194676>.
- Martínez-Rodríguez, Alejandro, María Martínez-Olcina, Manuel Vicente-Martínez, Nuria Asencio-Mas, Pau Navarro, Nuria Caturla, et Jonathan Jones. « Effectiveness of a Polyphenol-Enriched Blend on Weight Management and Metabolic Syndrome-Related Parameters in Healthy Overweight Adults ». *Applied Sciences* 14, no 9 (janvier 2024): 3882. <https://doi.org/10.3390/app14093882>.
- Martínez-Rodríguez, Alejandro, Lorena Vidal-Martínez, María Martínez-Olcina, Laura Miralles-Amorós, Juan Antonio Sánchez-Sáez, Domingo Jesús Ramos-Campo, Javier Sánchez-Sánchez, et al. « Study the Effect of an Innovative Educational Program Promoting Healthy Food Habits on Eating Disorders, Mediterranean Diet Adherence and Body Composition in University Students ». *Healthcare* 11, no 7 (janvier 2023): 965. <https://doi.org/10.3390/healthcare11070965>.
- Mavisoy Ordoñez, Kevinn Andrey, et Cristian Daniel Mejía Morales. « Valor Predictivo de Bioimpedancia Sobre El Estado Nutricional de La Comunidad Académica de Dos Universidades Colombianas », 2022. <http://repository.unilibre.edu.co/handle/10901/26418>.
- Menegatti, Erica, Anselmo Pagani, Giampiero Avruscio, Marianna Mucignat, et Sergio Giancesini. « The Effects of Thermal Water Physical Exercise in Patients with Lower Limb Chronic Venous Insufficiency Monitored by Bioimpedance Analysis ». *Diagnostics* 10, no 11 (novembre 2020): 889. <https://doi.org/10.3390/diagnostics10110889>.
- Miralles-Amorós, Laura, Nuria Asencio-Mas, María Martínez-Olcina, Manuel Vicente-Martínez, José Manuel García-De Frutos, Marcelo Peñaranda-Moraga, Lucía González-Alvarado, Rodrigo Yáñez-Sepúlveda, Guillermo Cortés-Roco, et Alejandro Martínez-Rodríguez. « Study the Effect of Relative Energy Deficiency on Physiological and Physical Variables in Professional Women Athletes: A Randomized Controlled Trial ». *Metabolites* 13, no 2 (23 janvier 2023): 168. <https://doi.org/10.3390/metabo13020168>.
- Morcillo-Muñoz, Jorge A., Felipe Marulanda-Mejía, Clara H. González-Correa, Andrés F. Morcillo-Muñoz, Bernardo Uribe, et Juan C. Ibarra-Jurado. « Impact of sarcopenia in clinical and functional outcomes and dependency degree in stroke patients ». *The Journal of Latin American Geriatric Medicine* 8, no 1 (2022). [https://www.jgeriatricmedicine.com/frame\\_esp.php?id=68](https://www.jgeriatricmedicine.com/frame_esp.php?id=68).
- Neri, M, L Morales, et Y Becerril. « Agreement between the results of body composition analysis from two electrical bioimpedance devices ». *Journal of Physics: Conference Series* 3014, no 1 (1 mai 2025): 012033. <https://doi.org/10.1088/1742-6596/3014/1/012033>.
- Nezodet, Charlie, Joseph Gandrieau, Philippe Nguyen, et Gautier Zunquin. « Perceived Physical Literacy Is Associated with Cardiorespiratory Fitness, Body Composition and Physical Activity Levels in Secondary School Students ». *Children* 10, no 4 (avril 2023): 712. <https://doi.org/10.3390/children10040712>.
- Odabaş, İlhan, Lale Güler, et Ali Günay. « Evaluation of Body Mass Index and Body Compositions of Elite and Non-Elite Korfball Athletes by Gender: Descriptive-Comparative Study ». *Türkiye Klinikleri Journal of Sports Sciences* 14, no 1 (2022): 61-68. <https://doi.org/10.5336/sportsci.2021-86032>.
- Peñaloza-Talavera, Ma. Fidelina, Clara H. Gonzalez-Correa, William Narvaez-Solarte, Izabella C. Gomes-Santana-Pereira, et Jhony A. Diaz-Vallejo. « Comparative analysis of body composition results of university students obtained using two bioimpedance analyzers ». *Journal of Electrical Bioimpedance* 16, no 1 (s. d.): 56-61. <https://doi.org/10.2478/joeb-2025-0008>.
- Sánchez Acosta, Camila Andrea, Jonathan Fernando Vieda Yepes, et Cristian David Jaramillo. « Afectación metabólica del trabajo nocturno y por turnos en los recepcionistas del sector hotelero de Ibagué ». *Thesis, Corporación Universitaria Minuto de Dios, 2023*. <https://repository.uniminuto.edu/handle/10656/18460>.
- Stuck, A. K., A. Weber, R. Wittwer, A. Limacher, et R. W. Kressig. « Performance of a Novel Handheld Bioelectrical Impedance Device for Assessing Muscle Mass in Older Inpatients ». *The Journal of Frailty & Aging* 11, no 2 (2022): 156-62. <https://doi.org/10.14283/jfa.2021.40>.
- Tapasco-Tapasco, L. O., C. A. Gonzalez-Correa, et A. Letourneur. « Phase Angle and Impedance Ratio as Meta-Inflammation Biomarkers after a Colon Cleansing Protocol in a Group of Overweight Young Women ». *Physiological Measurement* 45, no 5 (mai 2024): 055021. <https://doi.org/10.1088/1361-6579/ad46df>.
- Touillaud, Marina, Baptiste Fournier, Olivia Pérol, Lidia Delrieu, Aurélie Maire, Elodie Belladame, David Pérol, et al. « Connected device and therapeutic patient education to promote physical activity among women with localised breast cancer (DISCO trial): protocol for a multicentre 2x2 factorial randomised controlled trial ». *BMJ Open* 11, no 9 (13 septembre 2021): e045448. <https://doi.org/10.1136/bmjopen-2020-045448>.
- Wekre, Stian Lande, Halvor Dagsøen Landsverk, Jacky Lautridou, Astrid Hjelde, Jean Pierre Imbert, Costantino Balestra, et Ingrid Eftedal. « Hydration status during commercial saturation diving measured by bioimpedance and urine specific gravity ». *Frontiers in Physiology* 13 (2022). <https://www.frontiersin.org/articles/10.3389/fphys.2022.971757>.

# Partners and user centers





## Literature notes

1. Khalil SF, Mohktar MS, Ibrahim F. The Theory and Fundamentals of Bioimpedance Analysis in Clinical Status Monitoring and Diagnosis of Diseases. *Sensors*. 2014;14(6):10895-10928. doi:10.3390/s140610895
2. Bellido D, Garcia-García C, Talluri A, Lukaski HC, Garcia-Almeida JM. Future lines of research on phase angle: Strengths and limitations. *Rev Endocr Metab Disord*. Published online April 12, 2023;1-21. doi:10.1007/s11154-023-09803-7
3. Tapasco-Tapasco LO, Gonzalez-Correa CA, Letourneur A. Phase angle and impedance ratio as meta-inflammation biomarkers after a colon cleansing protocol in a group of overweight young women. *Physiol Meas*. 2024;45(5):055021. doi:10.1088/1361-6579/ad46df
4. Kyle UG, Bosaeus I, De Lorenzo AD, et al. Bioelectrical impedance analysis--part I: review of principles and methods. *Clin Nutr Edinb Scotl*. 2004;23(5):1226-1243. doi:10.1016/j.clnu.2004.06.004
5. Kyle UG, Bosaeus I, De Lorenzo AD, et al. Bioelectrical impedance analysis-part II: utilization in clinical practice. *Clin Nutr Edinb Scotl*. 2004;23(6):1430-1453. doi:10.1016/j.clnu.2004.09.012
6. Cederholm T, Jensen GL, Correia MITD, et al. GLIM criteria for the diagnosis of malnutrition – A consensus report from the global clinical nutrition community. *Clin Nutr*. 2019;38(1):1-9. doi:10.1016/j.clnu.2018.08.002
7. Cruz-Jentoft AJ, Bahat G, Bauer J, et al. Sarcopenia: revised European consensus on definition and diagnosis. *Age Ageing*. 2019;48(1):16-31. doi:10.1093/ageing/afy169
8. Rubino F, Cummings DE, Eckel RH, et al. Definition and diagnostic criteria of clinical obesity. *Lancet Diabetes Endocrinol*. Published online January 2025:S2213858724003164. doi:10.1016/S2213-8587(24)00316-4
9. Donini LM, Busetto L, Bischoff SC, et al. Definition and Diagnostic Criteria for Sarcopenic Obesity: ESPEN and EASO Consensus Statement. *Obes Facts*. 2022;15(3):321-335. doi:10.1159/000521241
10. Mathisen TF, Ackland T, Burke LM, et al. Best practice recommendations for body composition considerations in sport to reduce health and performance risks: a critical review, original survey and expert opinion by a subgroup of the IOC consensus on Relative Energy Deficiency in Sport (REDs). *Br J Sports Med*. 2023;57(17):1148-1160. doi:10.1136/bjsports-2023-106812
11. Deurenberg P, Roubenoff R. Body Composition. *Intrad Hum Nutr MJ Gibney HH Vorster FJ Kok - SI Blackwell Publ* 2002. Published online January 1, 2009.
12. Kyle UG, Genton L, Karsegard L, Slosman DO, Pichard C. Single prediction equation for bioelectrical impedance analysis in adults aged 20–94 years. *Nutrition*. 2001;17(3):248-253. doi:10.1016/S0899-9007(00)00553-0
13. Kushner RF, Schoeller DA. Estimation of total body water by bioelectrical impedance analysis. *Am J Clin Nutr*. 1986;44(3):417-424. doi:10.1093/ajcn/44.3.417
14. Deurenberg P, Tagliabue A, Schouten FJ. Multi-frequency impedance for the prediction of extracellular water and total body water. *Br J Nutr*. 1995;73(3):349-358. doi:10.1079/bjn19950038
15. Kyle UG, Genton L, Hans D, Pichard C. Validation of a bioelectrical impedance analysis equation to predict appendicular skeletal muscle mass (ASMM). *Clin Nutr Edinb Scotl*. 2003;22(6):537-543. doi:10.1016/s0261-5614(03)00048-7
16. Espasa-Labrador J, Cebrián-Ponce Á, Galindo-López R, et al. Intra-rater reliability and agreement of a portable bioelectrical impedance analysis device for body composition assessment. *Measurement*. 2026;259:119550. doi:10.1016/j.measurement.2025.119550
17. Moonen HPFX, Van Zanten ARH. Bioelectric impedance analysis for body composition measurement and other potential clinical applications in critical illness. *Curr Opin Crit Care*. 2021;27(4):344-353. doi:10.1097/MCC.0000000000000840
18. Demirci C, Açı G, Demirci MS, et al. Impedance ratio: a novel marker and a powerful predictor of mortality in hemodialysis patients. *Int Urol Nephrol*. 2016;48(7):1155-1162. doi:10.1007/s11255-016-1292-1
19. Mulasi U, Kuchnia AJ, Cole AJ, Earthman CP. Bioimpedance at the bedside: current applications, limitations, and opportunities. *Nutr Clin Pract Off Publ Am Soc Parenter Enter Nutr*. 2015;30(2):180-193. doi:10.1177/0884533614568155
20. Barry VG, Peterson CM, Gower BA. Membrane Capacitance from A Bioimpedance Approach: Associations with Insulin Resistance in Relatively Healthy Adults. *Obes Silver Spring Md*. 2020;28(11):2184-2191. doi:10.1002/oby.22977
21. Garr Barry V, Chiang JL, Bowman KG, Johnson KD, Gower BA. Bioimpedance-Derived Membrane Capacitance: Clinically Relevant Sources of Variability, Precision, and Reliability. *Int J Environ Res Public Health*. 2022;20(1):686. doi:10.3390/ijerph20010686
22. Bartels EM, Sørensen ER, Harrison AP. Multi-frequency bioimpedance in human muscle assessment. *Physiol Rep*. 2015;3(4):e12354. doi:10.14814/phy2.12354
23. Yasutake K, Kumahara H, Shiose K, Kawano M, Michishita R. Association between grip strength and electrical properties measured by bioimpedance spectroscopy in women with dementia aged 77 to 97 years living in group homes. *Med Int*. 2024;4(4):33. doi:10.3892/mi.2024.157





[www.aminogram.com](http://www.aminogram.com)

AMINOGRAM SAS  
ATHELIA III – 96 Voie Atlas  
13600 La Ciotat – France  
[contact@aminogram.com](mailto:contact@aminogram.com)

Download  
the scientific  
journal

